Pregnancy Test Operating Instructions

CE 0123

This product is composed of the glass fiber strips of monoclonal antibody against human chorionic gonadotropin (hCG), anti-mouse IgG solid cellulose nitrate membrane and the bonders of absorptive colloidal gold - monoclonal antibody against hCG. It adopts the principles of double antibody sandwich method and immunochromatography to test the hCG in the urine.

Intended Use: used for early diagnosis of pregnancy
Contents: each pouch contains one test strip and one desiccant

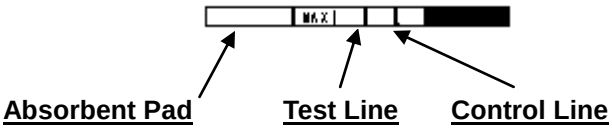

Test Procedure：
Before the use please prepare a timer and urine cup.

1. The Pregnancy test is formulated for use with fresh urine specimens. Urine cup should be used to collect specimens.
2. Remove the strip from the foil wrapper.
3. Immerse the strip into the urine with the arrow end pointing toward the urine. Do not cover the urine over the MAX (maximum) line. You may take the strip out after a minimum of 15 seconds in the urine and lay the strip flatly on a non-absorptive clean surface.
4. Read the result within 10 minutes.
5. Discard the test device after single use.

Interpretation of Results

Negative: If only one pink line appears in the control area, you can assume that you are not pregnant.
Positive: If two pink lines appear both in the control area and test area, you can assume that you are pregnant.
Inconclusive: If there is no distinct pink-purple colored band visible both in the TEST area and CONTROL area, the test is inconclusive. It is recommended that in this case the test should be repeated. If the problem persists, contact your local distributor.

Warnings & Precautions
For in vitro diagnostic use only

1. As with all diagnostic tests, a definitive diagnostic should not be based on the results of a single test, but should only be made by the physician after all clinical and lab findings have been evaluated.
2. Read directions for use carefully before performing this test. Pay attention to the position of the C and T line.
3. Do not use the kit beyond the labeled expiry date.
4. Do not reuse the test devices.
5. Do not use if pouch is damaged or opened.
6. Do not touch the membrane area.
7. Once open the pouch, the test device should be used immediately. Prolonged exposure to ambient humidity will cause product deterioration.

Distributed in the UK by: Home Health UK Ltd, Unit 11, Peerglow Industrial Estate, Olds Approach, Watford, Hertfordshire WD18 9SR. Website: http://www.homehealth-uk.com
Manufacturer: Nantong Egens Biotechnology Co. Ltd, Block A No.15 Building No. 1692, Xinghu Avenue, Nantong Economy & Technology Development Zone, Jiangsu Province P.R. China